

Page 199 bis

Add the following new figures 50 and 51:

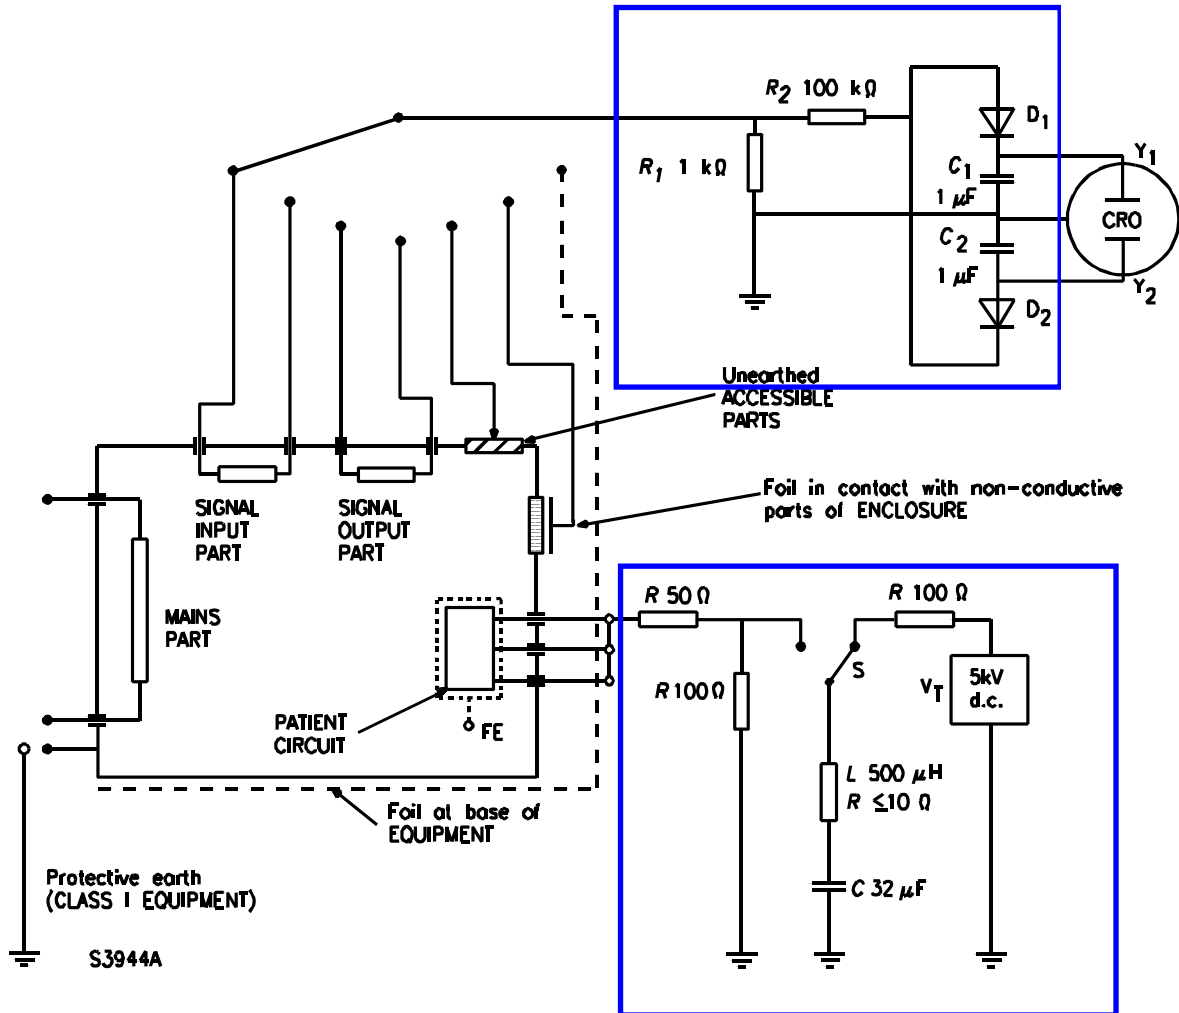


Figure 50 – Application of test voltage to bridged PATIENT CONNECTIONS for DEFIBRILLATION-PROOF APPLIED PARTS (see subclause 17 *h))